



[www.jbctools.com](http://www.jbctools.com)

Product  
website



## INSTRUCTION MANUAL



# SB05CC


5cc Syringe Barrel

This manual corresponds to the following reference:


**SB05CC**

# Packing List

The following items are included:

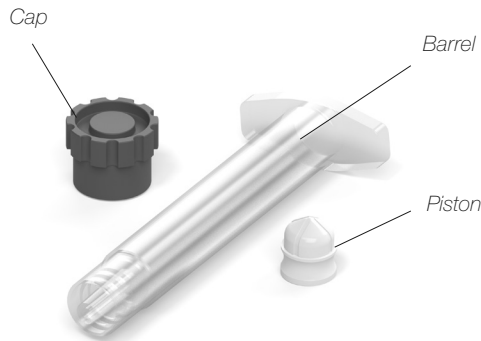

<b>5cc Syringe Barrel</b> .....	5 units
Ref. SB05CC	
includes (5 units each):	
<b>Barrel</b> Ref. 0029409	
<b>Piston</b> Ref. 0029414	
<b>Cap</b> Ref. 0029407	




<b>Manual</b> .....	1 unit
Ref. 0027371	

## Operation


SB05CC syringes are designed to be used with JBC DPM\* Manual Solder Paste Dispenser, ND-KS\* needles and ND-KP\* tapered tips.

### 1. Barrel Filling

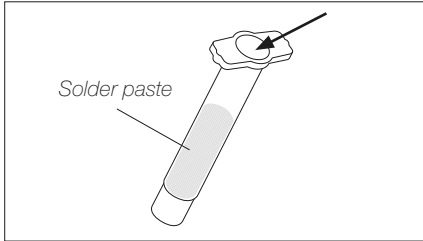


Fill in the syringe barrel with solder paste.

### 2. Piston Placement

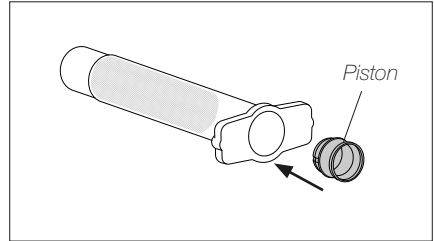

Fit the piston into the barrel.


### 3. Plunger Placement

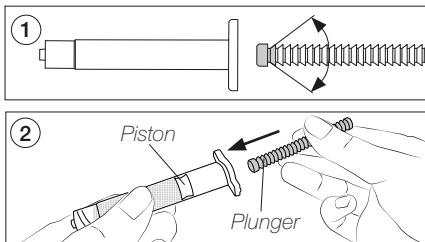

1. Note that the plunger enters with its head forward in the syringe barrel and the direction of the teeth angle corresponds to the upper image. Otherwise, DPM will not work properly.

2. Insert the plunger into the piston and press the piston against the solder paste to remove the air inside the barrel.

### 4. Tip Placement

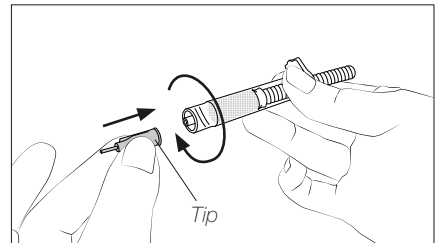

Screw the tip\* onto the syringe barrel.

\* More information on [www.jbctools.com](http://www.jbctools.com).

# Specifications

**SB05CC**

**Syringe Barrel**

Ref.: **SB05CC**

- Volume Capacity: 5 cc / 0.17 fl oz
- Weight: 0.02 kg / 0.04 lb
  
- Total Package Dimensions / Weight: 90 x 55 x 40 mm / 0.03 kg  
(L x W x H) 3.54 x 2.17 x 1.57 in / 0.07 lb

Complies with CE standards.  
ESD Safe.



**Warranty**

JBC's 2 year warranty covers this equipment against all manufacturing defects, including the replacement of defective parts and labor.

Warranty does not cover product wear or misuse.

In order for the warranty to be valid, equipment must be returned, postage paid, to the dealer where it was purchased.



This product should not be thrown in the garbage.  
In accordance with the European directive 2012/19/EU, electronic equipment at the end of its life must be collected and returned to an authorized recycling facility.

